



**0010-A35
SOUND LEVEL METER
OPERATION MANUAL**

PLEASE SCAN QR CODE TO
WATCH THE OPERATION
VIDEO OF PRODUCTS.



Safety Information

Read the following safety information carefully before attempting to operate or service the meter, and pls use the meter as specified in this manual:

● **Environmental conditions**

1. Altitude below 2000 meters
2. Relatively humidity 90% max
3. Operation Ambient 0~40°C

● **Maintenance & Clearing**

1. Repairs or servicing not covered in this manual should only be performed by qualified personnel
2. Periodically wipe the case with a dry cloth. Do not use abrasives or solvents on this instruments


General Description

This Sound Level Meter is designed to meet, the measurement requirements of Noise engineering, sound quality control, Health, Industrial safety offices in various environments. Such as factory, school, office and traffic lines.

- MAX/MIN measurement
- Over range indicate
- Low range indicate
- A&C weighting selection
- Bluetooth communication

Meter Description

- 1-LCD Display
- 2-Body of Meter
- 3-Microphone
- 4-HOLD/☼ button
- 5-MAX/MIN button
- 6-Power on/off button
- 7-UNITS button
- 8-Bluetooth button

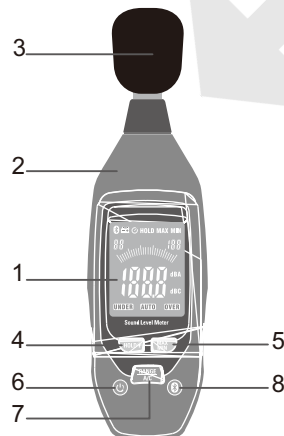

Button Discription

● **Power on/off, Auto-power off:**

Power on: Short press button to “☼” power on, system default auto power off. Long press to power on and disable auto power off function. Long press the button again to enable the auto power off function.

Power off: Short press button “☼” to power off

Auto-power off: Auto-power off signal “☼” displays in the left corner of LCD and the instrument will auto-power off in 10 minutes of no button operations.

If press the power on/off button for over 1 minutes, it will be recognized as faulty operation and the instrument will auto power off.

● **RANGE/(A/C) button:** Short press to switch range gear; Long press to switch unit.

● **☼ button:** Long press to active or deactivate Bluetooth.

● **HOLD/☼ button:** Short press to hold the current data; Long press to activate or deactivate backlight.

● **MAX/MIN button:** Press to record Maximum, Minimum

Note: MAX/MIN button, range button and A/C button will be deactivated when hold the current readings and the instrument will exit MAX/MIN recording function when switch range gear.

Display Layout

- ☼ : Bluetooth symbol
- ☼ : Low battery indicate
- ☼ : Timing power off symbol

MAX: Maximum hold

MIN: Minimum hold

Two smaller digits at upper left of display: Minimum range

Three smaller digits at upper right of display: Maximum range

UNDER: under range

OVER: over range

dBA, dBC: A-weighting, C-weighting.

AUTO: Auto range selection

HOLD: Data hold function

Four larger digits in middle of display: Measurement data



Operation instructions

Measurement Operation

- Turn on the instrument by pressing power on/off button.
- Short press button “RANGE” and select suitable measurement range based on no “UNDER” or “OVER” display on LCD.
- Select “dBA” for general noise sound level and “dBC” for measuring sound level of acoustic material.
- Hold the instrument in hand or fix it on tripod, take measure ata distance of 1~1.5 meters between microphone and source.

Data Hold

- Press hold button to freeze the readings and “HOLD” symbol displays LCD. Press hold button again to return normal measurement.

MAX/MIN reading

- Press MAX/MIN button for the first time, the instrument will enter Max tracking mode, the tracked max reading will display on the LCD.
- Press MAX/MIN button for the second time, the instrument will enter Min tracking mode, the tracked min reading will display on the LCD.
- Press MAX/MIN button for the third time, the current reading will display on the LCD.


Bluetooth communication

Long press Bluetooth button to activate Bluetooth function, it communicates after connect with the software. The instrument can transmit measured datas and instrument status to software and the software can control the instrument.

DataRecorder Operation



Download “INSIZE DataRecorder” APP to the mobile phone before using the Bluetooth communication function. Search the APP name “INSIZE DataRecorder” at APP Store (for IOS) or scan the QR code (for android) to download the APP.



Note: The instrument will automatically turn off in order to lengthen the battery working life. When symbol  appears on the LCD, pls replace the old battery with new ones.

- Open the battery compartment with a suitable screwdriver.
- Replace 9V battery.
- Mount the battery compartment again.

Specifications

Frequency range:	31.5Hz~8KHz
Accuracy:	±3.0dB (under reference condition of 94dB, 1kHz)
Range:	35~130dB
Measuring range:	LO: 35dB~80dB Med: 50dB~100dB Hi: 80dB~130dB Auto: 35dB~130dB
Frequency weighting:	A and C
Microphone:	1/2 inch electret condenser microphone
Digital display:	4 digits LCD display with a resolution: 0.1dB
Display Update:	2 times/sec
Auto power off:	Meter automatically shuts down after approx. 10 minutes of inactivity.
Power supply:	One 9V battery
Low battery indication:	The low battery signal “  ” flash when battery voltage drops below 7.2V; The backlight and low battery signal “  ” flash twice when battery voltage drops below 6.5V , then auto power off.
Operation temperature:	0°C~40°C/32°F~104°F
Operation humidity:	10%RH~90%RH
Storage temperature:	-10°C~+60°C/14°F~140°F
Storage humidity:	10%RH~75%RH
Weight:	184g
Dimensions:	185mmx54mmx36mm

Notice

- Do not store or operate the instrument at high temperature and high humidity environment.
- When not in use for long time, please take out the battery to avoid battery liquid leakage and cautery on the instrument.
- When using the instrument outdoors, pls mount thewindscreen on microphone in order to not pick up undesirable signals.
- Keep microphone dry and avoid severe vibration.